

1 **Evaluation of uncertainty sources in the determination of testosterone in urine by calibration-based and**
2 **isotope dilution quantification using ultra high performance liquid chromatography tandem mass**
3 **spectrometry**

4 J. Pitarch-Motellón, J. V. Sancho, M. Ibáñez, A. F. Roig-Navarro*. Research Institute for Pesticides and
5 Water, Universitat Jaume I, E-12071, Castelló, Spain. E-mail: roig@uji.es

6 N. Fabregat-Cabello. Department of Clinical Chemistry, University of Liège, Liège, Belgium

7 O. J. Pozo. Bioanalysis Research Group, IMIM, Hospital del Mar Medical Research Institute. Barcelona, Spain

8 Rosa Ventura, Barcelona Antidoping Laboratory, Doping Control Research Group, Fundació IMIM,
9 Barcelona, Spain. rventura@imim.es

10 JI García Alonso, Pablo Rodríguez-González, Adriana González Gago, Amaia Ereño Artabe. Department of
11 Physical and Analytical Chemistry, University of Oviedo, Oviedo, Spain.

12 Peter Van Eenoo, Koen Deventer. Ghent University, Department of Clinical Chemistry, Microbiology and
13 Immunology, Doping Control Laboratory, Zwijnaarde, Belgium.

14 Yvette Dehnes, Sebastian Rzeppa. Norwegian Doping Control Laboratory, Oslo University Hospital, Oslo,
15 Norway

16

17 **ABSTRACT**

18 Three quantification methodologies, namely calibration with internal standard (Cal-IS, non-weighted),
19 weighted calibration with internal standard (wCal-IS) and isotope pattern deconvolution (IPD) have been
20 used for the determination of testosterone in urine by LC-MS/MS. Uncertainty has been calculated and
21 compared for the three methodologies through intra- and inter-laboratory reproducibility assays. IPD
22 showed the best performance for the intra-laboratory reproducibility, with RSD and combined uncertainty
23 values below 4% and 9% respectively. wCal-IS showed similar performance, while Cal-IS where not constant
24 and clearly worse at the lowest concentration assayed (2 ng/mL) reaching RSD values up to 16%. The inter-
25 laboratory assay indicated similar results although wCal-IS RSD (20%) was higher than IPD (10%) and Cal-IS
26 get worse with RSD higher than 40% for the lowest concentration level. Uncertainty budgets calculated for
27 the three procedures revealed that intercept and slope were the most important factors contributing to
28 uncertainty for Cal-IS. The main factors for wCal-IS and IPD were the volumes of sample and/or standard
29 measured.

30

31 **INTRODUCTION**

32 The use of drugs to enhance performance in sports is a well-known and documented issue. Despite the
33 continuous introduction of new compounds, endogenous androgenic anabolic steroids (EAAS) are among
34 the most popular doping agents[1–3]. EAAS determination still represents an important challenge due to
35 the complexity to differentiate exogenous administration of endogenous substances. The goal requires
36 collaborative efforts as well as advanced methodologies[1–7]. Longitudinal fluctuations measurement for a
37 given athlete is nowadays regarded as the most effective approach to suspect the EAAS misuse. In this way,
38 the steroidal profile of the Athlete Biological Passport (ABP) represents a powerful tool to reveal doping
39 with endogenous compounds[1,3,6].

40 For most drugs, urine is the matrix generally used since it involves a non-invasive sampling procedure, large
41 volumes are easily obtained, shows wide time windows and concentrations are high enough[1,6,7].

42 However, sample preparation is mandatory to ensure matrix effect attenuation and good sensitivity and
43 selectivity. Usual treatment techniques such as solid phase extraction (SPE), liquid-liquid extraction (LLE)
44 and simple matrix dilution are normally used. Due to its simplicity, efficiency and low cost, LLE at basic pH is
45 still widely used in EAAS determination in urine samples[5,6]. Concerning identification and quantification,
46 LC-MS based techniques –equipped with Electrospray Ionization source (ESI)- tend to replace GC-MS(/MS) –
47 considered as the gold World Anti-doping Agency (WADA) standard for quantifications[8]- since the former
48 shows suitable sensitivity and faster instrumental run time. Specially UHPLC-MS/MS with its demonstrated
49 separation efficiency is considered the method of choice in doping analysis[1,5,6,9].

50 A relevant problem with the use of ESI source is the signal alteration due to matrix effect[10-12]. Matrix
51 effect can affect drastically to sensitivity, precision and accuracy of the analytical results. The most robust
52 approach to minimize matrix effect rely on the use of Stable Isotope Labeled-Internal Standard (SIL-
53 IS)[11,12]. Thus, matrix-effects associated to complex matrices can be properly overcome using a
54 quantification methodology based on isotope dilution mass spectrometry (IDMS). Classical IDMS is based
55 on the preparation of methodological calibration curves with the associated time consumption. An
56 alternative method of quantification, based on the measurement of isotopic abundances in the spiked
57 sample by multiple linear regression, can also be used. This method, known as isotope pattern
58 deconvolution (IPD), do not requires the construction of any calibration graph and has been tested
59 satisfactorily for rapid quantifications in different complex matrices[13-16]. IDMS together with IPD is a fast
60 and reliable methodology, which provides one result per injection with high accuracy and free of matrix
61 effect.

62 In the field of doping analysis, improvements of reliability and robustness of analytical results is
63 continuously and still required[1,2,5,6]. WADA highlights the need of good inter-laboratory precision,
64 particularly relevant in ABP profiling[5]. Analytical results for ABP are obtained from different laboratories
65 for the same athlete, thus, improving inter-laboratory precision seems of maximum concern to allow
66 universal application of any developed methodology. In this way, the need of calculating and minimizing
67 measurement uncertainty deserves to be treated thoroughly[2,17,18].

68 In the present work, a previously developed method has been applied to assess the uncertainty in the
69 testosterone concentration determined in several synthetic urine samples. Testosterone concentration has
70 been calculated using three different methodologies, weighted and non-weighted calibration with IS (wCal-
71 IS and Cal-IS, respectively) and IPD. In order to evaluate more in depth the associated uncertainty, an inter-
72 laboratory comparison among five laboratories has been performed. For all three methodologies, intra- and
73 inter-laboratory measurements have been conducted, combined uncertainties (u_c) and full uncertainty
74 budgets have been obtained and compared.

75

76 **EXPERIMENTAL**

77 **Reagents and materials**

78 Testosterone (T, purity 99%) was provided by Sigma-Aldrich Co. (Madrid, Spain) and $^{13}\text{C}_2$ -testosterone ($^{13}\text{C}_2$ -
79 T, purity 98% and $^{13}\text{C}_2$ -enrichment 98%) by Cambridge Isotope Laboratories (Andover, MA, USA).

80 Methanol (MeOH, HPLC quality) and methyl tert-butyl ether (MTBE, GC quality) were provided by Scharlau
81 (Barcelona, Spain). For the sample hydrolysis, β -glucuronidase from *E. coli* K12 provided by Roche
82 (Indianapolis, IN, USA) was employed. A 1 M phosphate buffer was prepared by dissolving the proper
83 amount of $(\text{NH}_4)_2\text{HPO}_4$ (Merck, Darmstadt, Germany) in Milli-Q water and adjusted to pH=7 with HCl 37%
84 from Scharlau (Barcelona, Spain). Also, a $\text{NaHCO}_3/\text{Na}_2\text{CO}_3$ (1:2, w/w) (Sigma-Aldrich Co., Madrid, Spain)

85 solid buffer was prepared. Formic acid (LC additive quality) and a 500 mM solution of NH₄HCOO (Scharlau,
86 Barcelona, Spain) in methanol HPLC were used for the mobile phase preparation.

87 A 250 µg/mL stock solution of T was prepared by dissolving 25 mg of solid standard, accurately weighed, in
88 100 mL of methanol. The stock solution of ¹³C₂-T was prepared by dissolving 10 mg of the purchased
89 material in 50 mL of methanol. This provided a concentration by reverse isotope dilution against the
90 natural compound of 237 µg/mL.

91 Individual 10 µg/mL and 1 µg/mL working solutions of the natural and labelled compounds were prepared
92 by dilution of the stock solutions with methanol. All of the standard solutions were stored in amber glass
93 bottles in a freezer.

94 The water purification system used was a Milli-Q gradient A10 from Millipore (Bedford, MA, USA).

95

96 Instrumentation

97 All participants in the inter-laboratory comparison have determined testosterone by LC-MS/MS.



98 Additionally some laboratories have used other methodologies (see inter-laboratory comparison section).

99 This section describes the instrumentation used at Research Institute for Pesticides and Water (IUPA)
100 laboratory, where the intra-laboratory measurements and all calculations have been done.

101 An Acquity UPLC system coupled to a TQD triple quadrupole mass spectrometer from Waters Corp.
102 (Milford, MA, USA) was employed for sample analysis. Chromatographic separation was performed with an
103 Acquity UPLC BEH C18 column (1.7 µm, 2.1 mm x 100 mm), also from Waters Corp., at a 0.3 mL/min flow
104 rate and an injection volume of 10 µL. The column oven was kept at 55°C and the sample manager at 10°C.
105 Mobile phase A was purified water and mobile phase B was MeOH HPLC, both containing 0.01% of formic
106 acid and 1 mM of NH₄HCOO as modifiers. The gradient applied was: 45% B (0-1 min), linear increase to
107 77.5% B in 6.5 min, 95% B (7.51-8 min), 45% B (8.5-11.5 min). Chromatograms of blank and a selected
108 sample can be seen in Figure S.8 in supplementary material.

109

110 Table 1. Chemical structure and experimental conditions of the LC-(ESI)-MS/MS for testosterone and
111 labeled testosterone

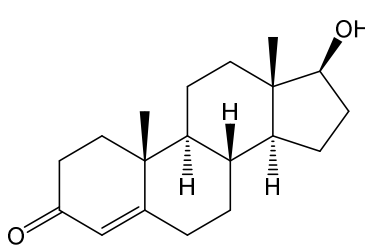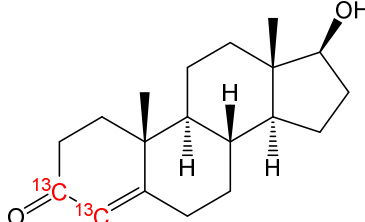Compound	Structure	Rt (min)	Precursor ion	Cone voltage (V)	SRM transitions
T		5.7	[M+H] ⁺	30	289.2 > 96.9 (25)
					290.2 > 96.9 (25)
					289.2 > 108.9 (25)
¹³ C ₂ -T		5.7	[M+H] ⁺	30	291.2 > 98.9 (25)
					292.2 > 98.9 (25)

112

113 Electrospray ionization in the mass spectrometer was performed at 120 °C and 350 °C source and
114 desolvation temperatures, 80 and 800 L/h cone gas and desolvation flow, respectively, and 3.5 kV capillary
115 voltage, operating in positive ion mode. MS/MS experimental conditions for T and ¹³C₂-T are listed in Table
116 1.

117 Nitrogen was employed as both drying and nebulizing gas, obtained from a nitrogen generator N₂ LC-MS
118 adapted for LC-MS analyzers (Claind, Teknokroma, Barcelona, Spain). Collision cell was operated under a
119 pressure of approximately 5.6 x 10⁻³ mbar of argon 99.995% (Praxair, Madrid, Spain). Dwell times of 0.1 s
120 per SRM transition were chosen. MassLynx v4.1 (Waters) and homemade Excel spreadsheets were used to
121 process the data obtained. Relative abundances of individual 100 ng/mL standards were determined (n=5)
122 under this conditions with RSD values under 1.5%.

123

124 **Sampling and sample preparation**

125 The aim of the study was explained to 15 healthy volunteers (8 men and 7 women with ages comprised
126 between 16 and 59 years) and consent was obtained after confirmation that they fully understood the
127 experiment. Urine samples were collected and stored at -20°C until use. Testosterone concentration was
128 approximately determined by IPD for all samples. 12 samples were selected and mixed in pairs in
129 approximate 1:1 (v/v) ratios to obtain 6 synthetic urine samples, A to F, with increasing concentrations
130 along the 2 ng/mL to 75 ng/mL testosterone range.

131 2.5 mL of the synthetic samples were transferred to individual glass tubes, together with 25 µL of 1 µg/mL
132 ¹³C₂-T, and they were neutralized with 1 mL of 1 M phosphate buffer (pH 7.0). Then, 30 µL of β-
133 glucuronidase solution were added. Samples were incubated at 55 ± 2 °C in a water bath for 1 h.

134 After hydrolysis, approximately 200 mg of a NaHCO₃/Na₂CO₃ (1:2, w/w) solid buffer were added and
135 dissolved by stirring in a vortex. Liquid-liquid extraction was performed with 6 mL of MTBE and stirring in a
136 vortex for 1 min. Separation of phases was achieved by centrifugation at 3500 rpm for 5 min and the upper
137 organic phase was transferred to clean glass tubes with disposable Pasteur pipettes, carefully avoiding to
138 transfer any aqueous phase. MTBE was evaporated in a MiVac at 40°C for 20 min. The residue was
139 reconstituted in 300 µL of MeOH/H₂O 1:1 (v/v) and transferred to LC vials.

140 Samples and standards were equally treated and analyzed as described above.

141

142

143 **Quantification methods**

144 The 6 synthetic urine samples (A to F) were analyzed by three quantification approaches: Cal-IS, wCal-IS and
145 IPD.

146 Additionally, at IUPA laboratory, standard addition was also employed for the inter-laboratory experiment.
147 On this purpose, 2.5mL aliquots of each sample were spiked with 0, 0.5, 2 and 3.5 times the original
148 approximate concentration of T and adjusted to a final volume of 2720 µL with water. The described
149 sample treatment was applied without the addition of internal standard.

150 For all participant laboratories, calibration curves freshly prepared consisted in 6 points between 0 and 100
151 ng/mL of T in 2.5mL of water. Using the same data acquired for calibration with IS, weighed calibration
152 calculations were applied as described in Garcia-Alonso and Rodríguez-González[19]. The weighing factor
153 used has been the common value inverse of the variance (1/SD²).

154 IPD was applied to the same sample extracts used in Cal-IS.

155 The isotope dilution quantification methodology employed is based on multiple linear regression and the
156 spiking of samples with an isotopically enriched analog of the analytes of interest. This produces an
157 intentional alteration of the natural isotopic composition of the analyte in the mix. Briefly, the altered
158 isotopic composition measured in the mixture $A_{mix}^{SRM_i}$ is a combination of the contribution of the
159 abundances of the natural, $A_{nat}^{SRM_i}$, and the isotopically enriched spike, $A_{lab}^{SRM_i}$ analyte. For a single
160 isotopically enriched spike and n measured transitions, this can be expressed in matrix notation as:

$$161 \begin{bmatrix} A_{mix}^{SRM1} \\ A_{mix}^{SRM2} \\ \vdots \\ A_{mix}^{SRMn} \end{bmatrix} = \begin{bmatrix} A_{nat}^{SRM1} & A_{lab}^{SRM1} \\ A_{nat}^{SRM2} & A_{lab}^{SRM2} \\ \vdots & \vdots \\ A_{nat}^{SRMn} & A_{lab}^{SRMn} \end{bmatrix} \begin{bmatrix} X_{nat} \\ X_{lab} \end{bmatrix} + \begin{bmatrix} e^{SRM1} \\ e^{SRM2} \\ \vdots \\ e^{SRMn} \end{bmatrix}$$

162 A vector error e^{SRM1} needs to be included in order to solve the system by multiple linear regression, which
163 gives the molar fractions of natural and labelled compounds (X_{nat} and X_{lab} respectively) as solutions.
164 These can be obtained in any spreadsheet software with a linear regression function (LINEST in Microsoft
165 Excel) inserting the data in matrix form. Then, since the added amount of labelled compound N_{lab} is
166 known, the amount of natural compound in the sample N_{nat} is readily calculated (Table S.4. Supplementary
167 information):

$$168 N_{nat} = N_{lab} \frac{X_{nat}}{X_{lab}}$$

169 As it can be seen, no methodological calibration procedures are required and a single injection provides
170 one concentration value of the sample. The mass isotopomer distribution from each precursor ion has to
171 be determined experimentally in the mix and compared with the individual distributions corresponding to
172 the natural and the labeled analyte, the reference distributions. These individual distributions can be
173 theoretically calculated or experimentally measured. In the present work, they have been experimentally
174 measured. In a first step, theoretical isotopomer distributions have been obtained by IsoPatrn software
175 implemented by L. Ramaley and L. Cubero-Herrera[20]. Afterwards, only those transitions producing
176 instrumental signal significantly different from background have been selected. A thorough description of
177 the general IPD methodology and its application to different analyte types can be found in the
178 literature[21-23].

179

180 **Inter-laboratory experiment**

181 For the inter-laboratory variability evaluation of both calibration and IPD methods, four laboratories were
182 contacted and agreed to collaborate: Barcelona Antidoping Laboratory (Fundació IMIM, Barcelona, Spain),
183 Doping Control Laboratory (DoCoLab, Ghent University, Ghent, Belgium), Norwegian Doping Control
184 Laboratory (Oslo University Hospital, Oslo, Norway) and the Department of Physical and Analytical
185 Chemistry at University of Oviedo (Oviedo, Spain).

186 Three plastic bags containing 12 mL of frozen samples A to F in individual Falcon tubes, a vial with 1 mL of
187 $^{13}\text{C}_2\text{-T}$ 10 $\mu\text{g}/\text{mL}$ in MeOH and Instructions and Results documents were prepared. The bags were put into
188 sealed packages with the required amount of dry ice to ensure sub-zero temperature conditions until
189 arrival to the selected laboratories. Samples were processed and all the required measurements were
190 performed in order to apply calibration and IPD calculations at our laboratory. In addition, laboratories
191 were also asked to perform any other routine quantification method they had implemented (Table 2).
192 Taking into account those extra quantification methods, we got 19 analytical results for each sample. These

193 results were used to calculate a consensus value for the concentration of each sample, C_{ref} , and its
194 associated uncertainty, u_{ref} .

195 Table 2. Additional quantification procedures conducted in inter-comparison participating laboratories

Laboratory	Additional analytical methods
IUPA	Standard additions (LC-MS/MS)
DoCoLab	GC-MS/MS, LC-HRMS
Norwegian Doping Control Laboratory	GC-MS/MS

196

197 **Uncertainty assessment**

198 In the present work, measurement of uncertainty was evaluated according to WADA technical document
199 TD2014DL [24] and references therein. Specifically the procedure based in the Nordtest guide [25]. To this
200 end, an intra-laboratory reproducibility experiment (five replicates of each sample along five weeks) and a
201 short inter-laboratory comparison have been conducted. Combined uncertainty, u_{comb} , for each selected
202 quantification method and sample were calculated and compared. Moreover, the inter-laboratory
203 reproducibility standard deviation was calculated and compared for the three selected methods. Combined
204 uncertainty has been calculated as:

205
$$u_{comb} = \sqrt{u_{SD}^2 + u_{bias}^2}$$

206 where u_{SD}^2 is the intra-laboratory reproducibility standard deviation for the five replicates obtained along
207 five consecutive weeks at IUPA laboratory and u_{bias} is the uncertainty associated to any source of bias which
208 accounts for the method and laboratory bias, including the uncertainty associated to the consensus
209 reference value. To that purpose, a short inter-laboratory comparison was conducted and a whole of 19
210 quantification results have been obtained for each sample A to F (see inter-laboratory experiment section).
211 Thus, u_{bias} was calculated as

212
$$u_{bias} = \sqrt{RMS^2 + u_{ref}^2}$$

213 where u_{ref} is the bias uncertainty associated to the consensus concentration value for each sample, C_{ref} ,
214 obtained by:

215
$$u_{ref} = \frac{S_R}{\sqrt{n}}$$

216 where S_R is the mean standard deviation for the inter-laboratory reproducibility and n is the number of
217 results for each sample. A $n=17$ was employed instead of 19 due to exclusion of outliers determined by
218 Hampel test (see results, Table 3 and Table S.7 from Supplementary Information).

219 RMS is the root mean square bias for each quantification method used in the intra-laboratory
220 reproducibility assessment conducted at IUPA lab (for examples of calculations see Table S.5 in
221 supplementary material).

222 For each sample (A to F) a mean bias has been calculated from the intra-lab reproducibility study ($n = 5$).
223 These mean bias have been used to calculate RMS as:

224
$$RMS = \sqrt{\frac{\sum_i bias_i^2}{6}}$$

225

226 On the other hand, contribution of any source of uncertainty to a given measurement, known as full
227 uncertainty budget, can be calculated using the Kragten approach [26]. Briefly, it consists in an
228 approximation of error propagation theory calculations adapted for its implementation in spreadsheet
229 programs (such as Microsoft's Excel). Calculation tables are constructed with all the parameters used to
230 obtain the final analytical result including their uncertainty or standard deviation. Then, parameter values
231 are sequentially altered with their SD to obtain the deviation (Δ^2) produced to the analytical result in
232 relation to the unchanged value, which constitutes the magnitude of contribution to total uncertainty of
233 the analytical procedure. It is readily calculated for each parameter i as:

$$234 \quad \Delta_i^2 = (x - x_i)^2$$

235 Where x is the unchanged value and x_i is the new value with one parameter altered. Then, total uncertainty
236 of the procedure ($U(x)$) can be obtained using:

$$237 \quad U(x) = \sqrt{\sum_i \Delta_i^2}$$

238 Examples of complete uncertainty calculations can be consulted in the Supplementary Information (Table
239 S.6).

240

241 **RESULTS AND DISCUSSION**

242 **IPD measurements**

243 As explained above, IPD calculations rely on the relative abundance distribution of natural and labelled
244 compounds and, therefore, on their accuracy. For this purpose, the most abundant SRM transitions for
245 each compound were selected with IsoPatrn software. Then, relative abundances were experimentally
246 determined by preparing individual 100 $\mu\text{g/L}$ standards in MeOH/H₂O 1:1 (v/v) and injecting them five
247 times each (Tables S.1 and S.2 in supplementary information). Mean values for experimental abundances
248 were used in subsequent quantification procedure and standard deviations were used in the uncertainty
249 budgets building procedure.

250 IPD calculation also requires to know the exact amount of labelled compound added to samples. Exact
251 concentration of the ¹³C₂-T working standard solution was calculated by reverse isotope dilution (RID)
252 against the natural T solution, resulting in 12.20 ± 0.10 mg/L. (Table S.3 supplementary information).

253

254 **Evaluation of uncertainty**

255 Uncertainty has been assessed as intra-laboratory reproducibility standard deviation and through the
256 reproducibility of an inter-laboratory comparison.

257 Intra-laboratory has been conducted at IUPA facilities. Five replicates of the synthetic urine samples (A to F)
258 have been analyzed along five consecutive weeks. Concentration mean values, as well as standard
259 deviation and RSD(%) are shown in Table 3.

260 Regarding intra-lab precision, wCal-IS shows RSD below 5% for any concentration level. IPD quantification
261 performs slightly better while Cal-IS clearly achieves the worst reproducibility at the lower concentrations,
262 reaching a value of 15.8 % at 2 ppb level. Concerning the inter-laboratory comparison, results are
263 qualitatively similar. IPD shows the highest precision, with a mean RSD value around 10%, while wCal-IS
264 doubles that value. On the other hand, Cal-IS shows the worst performance at the lowest levels, where RSD
265 reaches values higher than 40%.

266

267 Table 3. Intra-laboratory and inter-laboratory precision data for the three quantification methodologies
268 assayed and for the consensus value. Cal_IS: non-weighted calibration with internal standard; w-Cal_IS:
269 weighted calibration with internal standard; IPD: isotope pattern deconvolution.

Sample	Mean ± SD (RSD%) ng/mL						
	Intra-lab reproducibility (n=5) ^a			Inter-lab reproducibility (n=5) ^b			Consensus C _{ref} (n=17) ^c
	Cal_IS	w-Cal_IS	IPD	Cal_IS	w-Cal_IS	IPD	
A	1.9 ± 0.3 (15.8)	2.04 ± 0.06 (2.9)	2.10 ± 0.04 (1.9)	2.1 ± 0.9 (43)	2.2 ± 0.4 (18)	2.3 ± 0.3 (13)	2.0 ± 0.4 (20)
B	3.6 ± 0.3 (8.3)	3.78 ± 0.14 (3.7)	3.87 ± 0.06 (1.6)	4.1 ± 1.0 (24)	4.2 ± 0.8 (19)	4.3 ± 0.4 (9.3)	4.0 ± 0.4 (10)
C	10.1 ± 0.4 (4.0)	10.3 ± 0.5 (4.9)	10.48 ± 0.22 (2.1)	11.2 ± 1.9 (17)	11.6 ± 2.3 (20)	11.6 ± 0.9 (7.8)	11.2 ± 1.2 (11)
D	17.1 ± 0.9 (5.3)	17.4 ± 0.8 (4.6)	17.7 ± 0.6 (3.4)	19.5 ± 2.3 (12)	20 ± 4 (20)	20.3 ± 2.2 (11)	20 ± 3 (15)
E	51.7 ± 1.3 (2.5)	52.0 ± 1.1 (2.1)	52.9 ± 0.9 (1.7)	57 ± 8 (14)	60 ± 13 (22)	60 ± 5 (8.3)	57 ± 6 (11)
F	67.8 ± 1.9 (2.8)	68.0 ± 1.6 (2.4)	69.2 ± 0.9 (1.3)	75 ± 9 (12)	77 ± 16 (21)	78 ± 7 (9.0)	76 ± 10 (13)


270 ^a Results from IUPA laboratory

271 ^b One result from each of the five participant laboratories

272 ^c Consensus value calculated as the mean value for the results obtained from all quantification methodologies used in
273 the interlaboratory comparison. Outlier values were excluded following Hampel test (Table S.7). Associated bias
274 uncertainty of C_{ref} (U_{ref}) calculated from the Mean RSD% is 3.1% (see Table S.5)

275

276

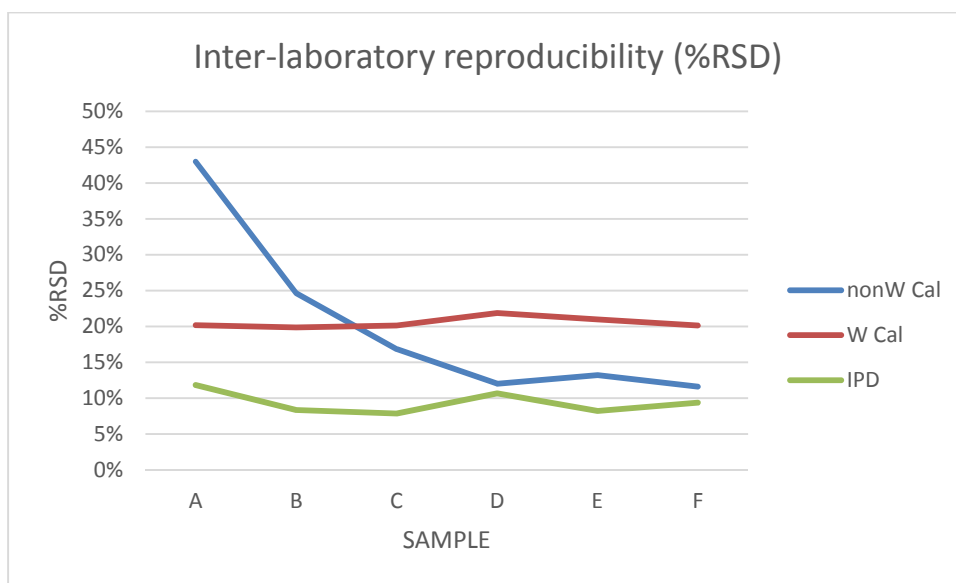

277

278 Figure 1. Mean inter-laboratory RSD values for the three quantification methods assayed. Concentration
279 ranges from 2 ng/mL (sample A) to 70 ng/mL (sample F).

280

281 Thus, inter-laboratory reproducibility noticeably shows tendencies with concentration (Figure 1). Cal-IS
282 performs poorly at low concentrations, with RSD > 40% in sample A, which decreases to values near 12% as
283 concentrations get higher. In comparison, wCal-IS provided constant values of RSD along the concentration
284 range (20%), improving uncertainty at low concentrations but performing slightly worse in the rest of the
285 samples. IPD produced significantly lower dispersion of values resulting in the highest inter-laboratory
286 precision (from 7.8% to 13%) of the three methods even at low concentrations.

287 In addition to intra-laboratory reproducibility, combined uncertainty, u_c , were calculated in order to
 288 estimate the measurement uncertainty for the three quantification methods. To this end, method and
 289 laboratory bias were estimated, according to the Nordtest guide [25] (see experimental), as the square root
 290 of two components: the percentage of the mean difference (RMS_{bias}) from a reference value (C_{ref}), and
 291 uncertainty of this reference value, u_{ref} . The end value for u_c accounts for the method and laboratory bias
 292 together with standard deviation of reproducibility at each concentration assayed (A-F samples) (Table 4).

293

294 Table 4. Combined uncertainty for the three quantification methodologies assayed.

Sample	Combined uncertainty (%)		
	Cal_IS	w-Cal_IS	IPD
u_{ref}		3.1%	
RMS_{bias}	10.4%	8.3%	6.9%
u_{bias}	10.9%	8.8%	7.6%
A	17.9%	9.4%	7.8%
B	13.2%	9.6%	7.8%
C	11.7%	10.0%	7.9%
D	12.0%	10.0%	8.4%
E	11.2%	9.1%	7.8%
F	11.3%	9.1%	7.7%

295

296 The consensus values obtained from the inter-laboratory comparison were adopted as reference values
 297 (Table 3). The consensus values are not intended to be used as certified values, but they were accepted as
 298 reference values to calculate bias uncertainty for each quantification methodology and to assess the bias
 299 associated to that reference value. A u_{ref} of 3.1% was obtained from the mean RSD value (12.9%) and $n=17$
 300 from the 19 quantification procedures applied minus outlier values (see experimental section and
 301 Supplementary Information for details).

302 Since the data required for Cal-IS and wCal-IS is exactly the same, taking into account the difference in
 303 combined uncertainty (11.2%-17.9% versus 9.1-10.0%) it is worth noting the improved quality of analytical
 304 results due only to the data treatment.

305 Along with wCal-IS, IPD stands out in comparison with more extensively used methods such as Cal-IS.
 306 Furthermore, IPD also provided combined uncertainties below 8.4% in all the concentration range with the
 307 advantage of reduced time analysis, since no calibration curve procedure had to be performed.

308 Again, results showed that Cal-IS performs poorly at low concentrations, being the worse method for the
 309 whole concentration range studied. In comparison, wCal-IS provided constant values of combined
 310 uncertainty along the concentration range although higher than IPD, which produced the lowest combined
 311 uncertainties of the three methods at any concentration assayed. This is in accordance with the high
 312 metrological quality of analytical results provided by isotope dilution mass spectrometry
 313 determinations[21].

314 Finally, full uncertainty budgets were obtained for the three selected quantification methods according to
 315 the Kragten approach (Table S.6 in supplementary material).


316 In the case of both wCal-IS and Cal-IS methods, the same 6 parameters were considered, including:
 317 intercept and slope of the linear regression, measurement of the area ratio in the sample (between natural

318 and labelled compound chromatographic peak areas, Rm), volume of sample (V_s), volume of internal
319 standard (V_t) and concentration of the natural standard (C_n). Calculations of the contribution of each
320 parameter to total procedure uncertainty were carried out for the five replicates and the average values
321 were obtained.

322 As it can be seen in Figure 2, in the case of Cal-IS, uncertainty contribution coming from the intercept of the
323 regression is predominant at low concentrations (Sample A) while at high concentrations (Sample F) slope
324 is the highest contributor to final method uncertainty. Thus, uncertainty for a Cal-IS method will hardly
325 improve experimentally. Probably, an alternative way to correct bias and its associated uncertainty at low
326 concentrations could be the use of a single external calibration point forced through the origin, an
327 approach not tested in the present work. In contrast, when using weighted calibration, the major
328 contributors to uncertainty were the measurement of sample and internal standard volumes. Thus, one
329 way to easily reduce uncertainty could be consider the mass instead of volumes.

330 On the other hand, the parameters considered for uncertainty calculations in IPD quantification were the
331 following: determination of abundances of the natural testosterone ($natT-1$, $natT-2$) and $^{13}C_2$ -testosterone
332 ($labT-1$, $labT-2$) transitions, measurement of those transitions in the sample blend ($B-1$, $B-2$, $B-3$, $B-4$),
333 volume of sample (V_s) and volume and concentration of $^{13}C_2$ -testosterone standard added (V_t , C_t).

334 As it might be expected for an isotope-dilution determination[21], one of the most important parameters in
335 IPD was the volume of labelled compound added to perform the quantification. As said above, this
336 contribution to uncertainty could be minimized by weighting the amount of solution added. Moreover, the
337 measurement of relative abundances in the sample blend, especially the most abundant transitions of
338 natural ($B-1$: 289 > 97) and labelled compounds ($B-3$: 291 > 99), contributed significantly to the final
339 uncertainty with relative magnitudes from 8.6% to 50%.

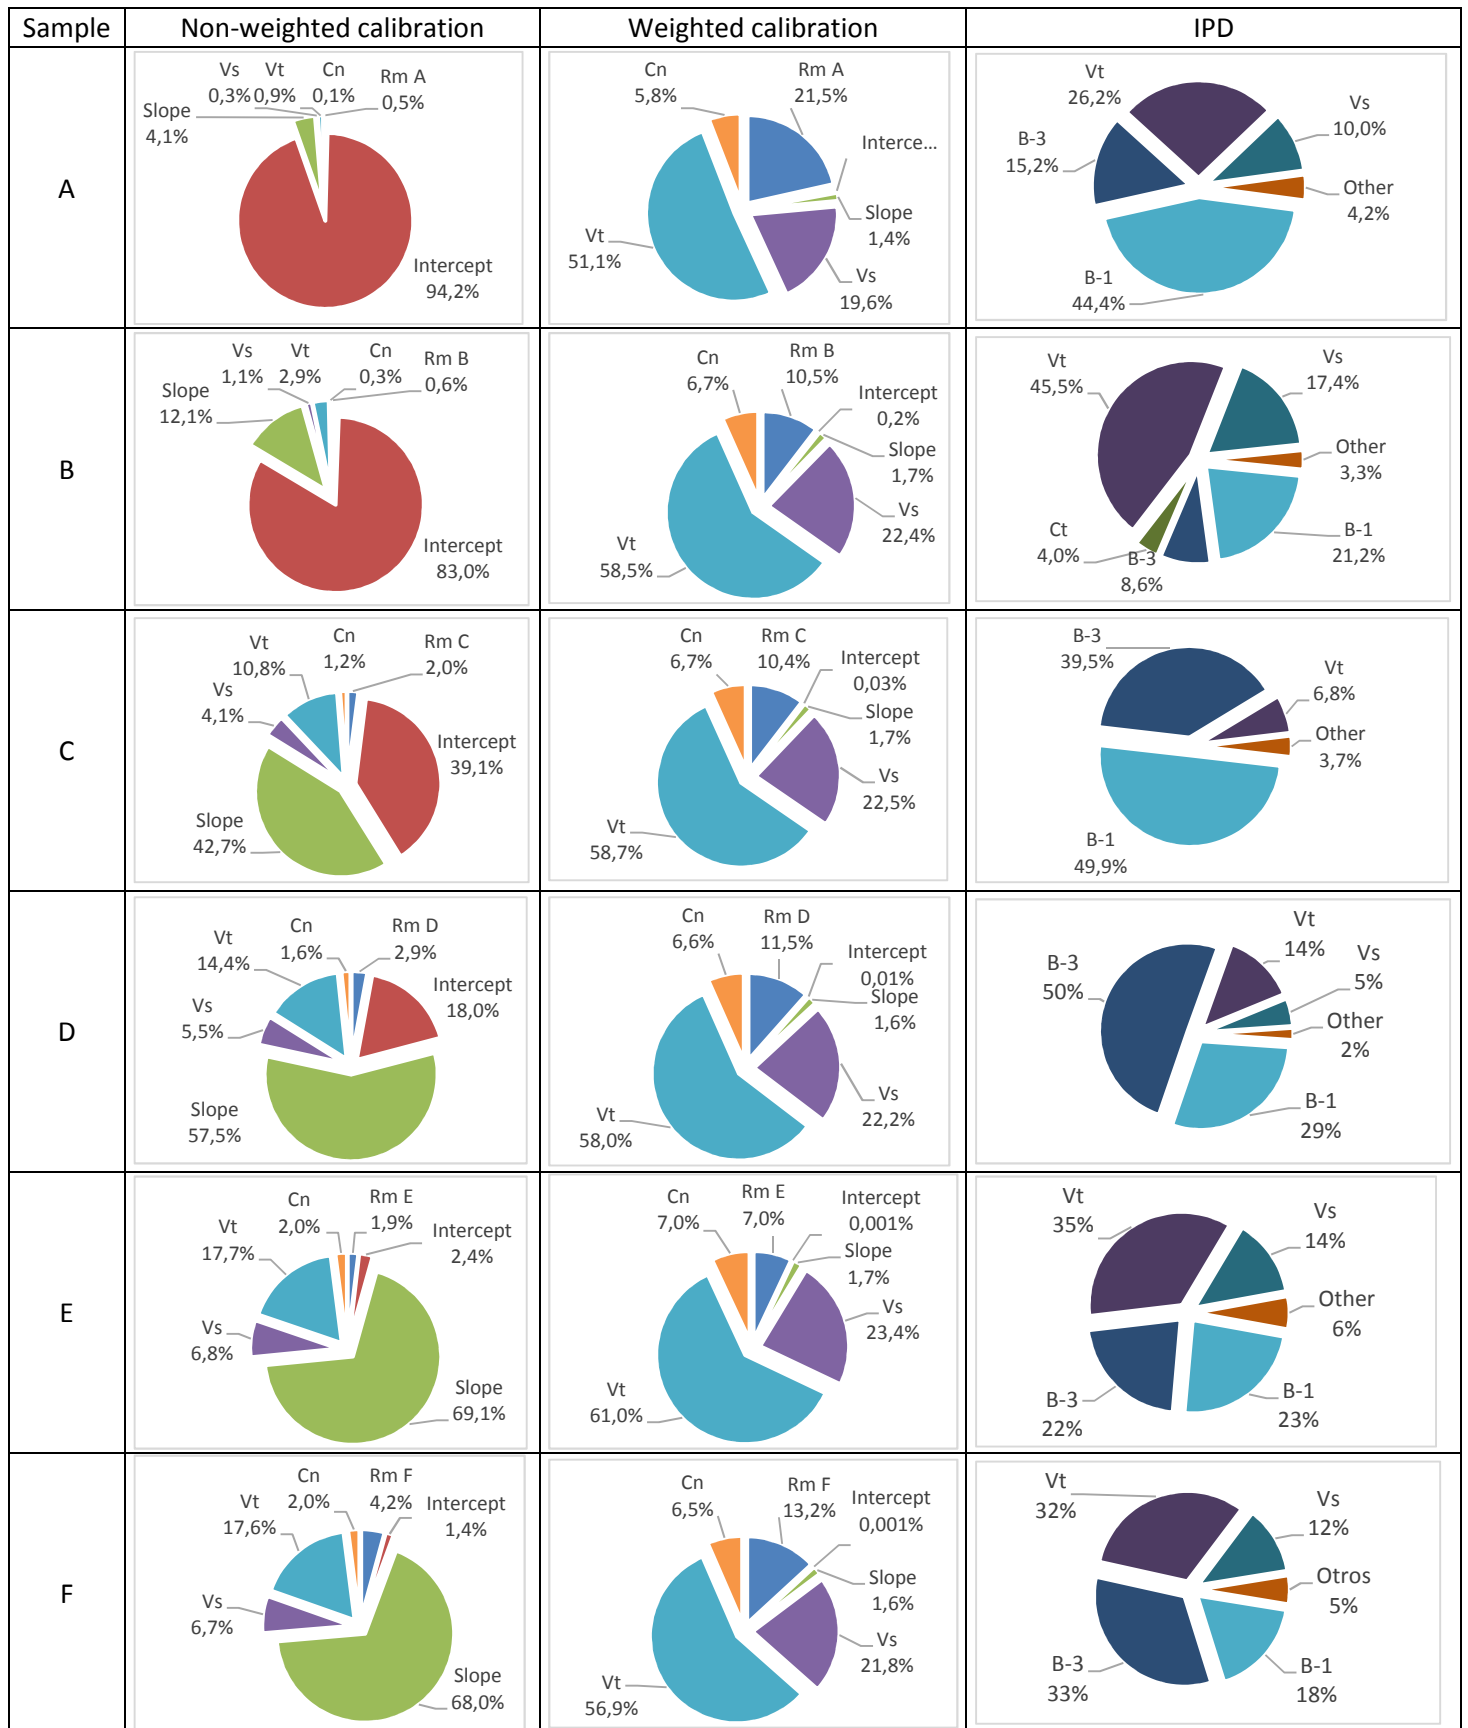

341

342 Figure 2. Uncertainty budgets for the quantification methods assayed.

343

344 **CONCLUSIONS**

345 In this work, three analytical approaches for the determination of testosterone in urine have been
346 compared from an uncertainty evaluation point of view.

347 Firstly, method uncertainty derived from the procedure itself has been evaluated at our laboratory by
348 applying weighted and non-weighted calibration with internal standard and IPD quantifications to 6
349 synthetic urine samples, composed of mixed human urine samples, in five different weeks. Inter-day
350 combined uncertainties for each sample and method were obtained by Nordtest calculation method and
351 showed similar values for weighted calibration and IPD, below or equal to 10% in all cases, while non-
352 weighted calibration yielded uncertainties ranging from 11.2% to 17.9%.

353 Secondly, an inter-laboratory experiment was carried out in order to set a reference value for the samples
354 and to further evaluate inter-laboratory RSD of these three methods. Similarly to the intra-laboratory
355 experiment, non-weighted calibration presented much higher uncertainty at low concentrations (43%) than
356 at medium and high concentrations (12%-24%), where it showed a better performance than weighted
357 calibration (18%-21% along all the range). In contrast, the combined uncertainty associated with IPD
358 method was lower than the other two in all 6 samples, ranging from 7.8% to 13%.

359 In addition, Kragten method was applied to intra-laboratory data to obtain the uncertainty budgets for the
360 considered quantification methods. Thus, linear regression parameters –slope and intercept– were found
361 to be the major contributors to uncertainty in non-weighted calibration, varying along the concentration
362 range. In contrast, weighted calibration and IPD methods were more stable in terms of relative
363 contributions to procedure uncertainty.

364 Hence, it has been demonstrated that weighted calibration might be more precise than classical calibration
365 with internal standard, providing similar uncertainties and standard deviations than isotope dilution
366 methodologies in intra-laboratory reproducibility studies. Moreover, the present IPD methodology yielded
367 lower inter-laboratory variability and thus, higher metrological quality of the analytical results are
368 expected.

369 The results presented in this work for testosterone as a model compound, together with the benefits of
370 reduced time analysis and matrix effect corrections provided by IDMS-based methodologies, highlights IPD
371 as a rapid, robust and reliable method. Thus, taking into account the lower uncertainty of the present
372 analytical approach, IPD is shown as a promising alternative to improve longitudinal fluctuations in steroid
373 profiling.

374

375 **ACKNOWLEDGEMENTS**

376 The authors acknowledge financial support from the Generalitat Valenciana (Research group of excellence
377 Prometeo II 2014/023 and Collaborative Research on Environment and Food Safety ISIC/2012/016), as well
378 as University Jaume I for project PB1-1B2013-55. Finally, the authors are grateful to the Serveis Centrals
379 d'Instrumentació Científica (SCIC) of University Jaume I for using Acquity and TQD instruments.

380

381

382

383 **REFERENCES**

- 384 [1] F. Gosetti, E. Mazzucco, M.C. Gennaro, E. Marengo, Ultra high performance liquid chromatography
385 tandem mass spectrometry determination and profiling of prohibited steroids in human biological
386 matrices. A review, *J. Chromatogr. B.* 927 (2013) 22–36. doi:10.1016/j.jchromb.2012.12.003.
- 387 [2] F. Botrè, New and old challenges of sports drug testing, *J. Mass Spectrom.* 43 (2008) 903–907.
388 doi:10.1002/jms.1455.
- 389 [3] A. Jarek, K. Kowalczyk, P. Chołbiński, K. Chajewska, E. Turek-Lepa, A. Pokrywka, E. Bulska, D.
390 Kwiatkowska, Analytical procedure for steroid profiling valid for Athlete Biological Passport, *Chem.*
391 *Pap.* 69 (2015) 254–261. doi:10.1515/chempap-2015-0030.
- 392 [4] C. Saudan, Testosterone and doping control, *Br. J. Sports Med.* 40 (2006) i21–i24.
393 doi:10.1136/bjism.2006.027482.
- 394 [5] F. Badoud, D. Guillarme, J. Boccard, E. Grata, M. Saugy, S. Rudaz, J.-L. Veuthey, Analytical aspects in
395 doping control: Challenges and perspectives, *Forensic Sci. Int.* 213 (2011) 49–61.
396 doi:10.1016/j.forsciint.2011.07.024.
- 397 [6] R. Nicoli, D. Guillarme, N. Leuenberger, N. Baume, N. Robinson, M. Saugy, J.-L. Veuthey, Analytical
398 Strategies for Doping Control Purposes: Needs, Challenges, and Perspectives, *Anal. Chem.* 88 (2016)
399 508–523. doi:10.1021/acs.analchem.5b03994.
- 400 [7] G.J. Trout, R. Kazlauskas, Sports drug testing - an analyst's perspective, *Chem. Soc. Rev.* 33 (2004) 1.
401 doi:10.1039/b201476a.
- 402 [8] World Anti-Doping Agency, WADA Technical Document – TD2016EAAS, (2016) 1–16.
- 403 [9] M. Thevis, A. Thomas, V. Pop, W. Schänzer, Ultrahigh pressure liquid chromatography–(tandem)
404 mass spectrometry in human sports drug testing: Possibilities and limitations, *J. Chromatogr. A.* 1292
405 (2013) 38–50. doi:10.1016/j.chroma.2012.12.048.
- 406 [10] P.J. Taylor, Matrix effects: the Achilles heel of quantitative high-performance liquid chromatography–
407 electrospray–tandem mass spectrometry, *Clin. Biochem.* 38 (2005) 328–334.
408 doi:10.1016/j.clinbiochem.2004.11.007.
- 409 [11] A. Furey, M. Moriarty, V. Bane, B. Kinsella, M. Lehane, Ion suppression; A critical review on causes,
410 evaluation, prevention and applications, *Talanta.* 115 (2013) 104–122.
411 doi:10.1016/j.talanta.2013.03.048.
- 412 [12] H. Trufelli, P. Palma, G. Famiglini, A. Cappiello, An overview of matrix effects in liquid
413 chromatography-mass spectrometry, *Mass Spectrom. Rev.* 30 (2011) 491–509.
414 doi:10.1002/mas.20298.
- 415 [13] A. González-Antuña, P. Rodríguez-González, G. Centineo, J.I. García Alonso, Evaluation of minimal
416 ¹³C-labelling for stable isotope dilution in organic analysis, *Analyst.* 135 (2010) 953.
417 doi:10.1039/b924432h.
- 418 [14] N. Fabregat-Cabello, J. Pitarch-Motellón, J. V. Sancho, M. Ibáñez, A.F. Roig-Navarro, Method
419 development and validation for the determination of selected endocrine disrupting compounds by
420 liquid chromatography mass spectrometry and isotope pattern deconvolution in water samples.

- 421 Comparison of two extraction techniques, *Anal. Methods*. 8 (2016) 2895–2903.
422 doi:10.1039/C6AY00221H.
- 423 [15] N. Fabregat-Cabello, P. Zomer, J.V. Sancho, A.F. Roig-Navarro, H.G.J. Mol, Comparison of approaches
424 to deal with matrix effects in LC-MS/MS based determinations of mycotoxins in food and feed, *World*
425 *Mycotoxin J.* 9 (2016) 149–161. doi:10.3920/WMJ2014.1872.
- 426 [16] N. Fabregat-Cabello, J. V Sancho, A. Vidal, F. V González, A.F. Roig-Navarro, Development and
427 validation of a liquid chromatography isotope dilution mass spectrometry method for the reliable
428 quantification of alkylphenols in environmental water samples by isotope pattern deconvolution., *J.*
429 *Chromatogr. A.* 1328 (2014) 43–51. doi:10.1016/j.chroma.2013.12.077.
- 430 [17] E. Spirito, F. Botre, The role of measurement uncertainty in doping analysis, *Int. J. Risk Assess.*
431 *Manag.* 5 (2005) 374. doi:10.1504/IJRAM.2005.007178.
- 432 [18] O. Barroso, J. Miller, A. Squirrell, S. Westwood, Measurement uncertainty in anti-doping quantitative
433 analysis for prohibited threshold substances, *Bioanalysis*. 4 (2012) 1653–1665.
434 doi:10.4155/bio.12.127.
- 435 [19] J.I. García-Alonso, P. Rodríguez-González, Uncertainty evaluation in IDMS, in: *Isot. Dilution Mass*
436 *Spectrom.*, RSC Publishing, 2013: pp. 379–433
- 437 [20] L. Ramaley, L.C. Herrera, Software for the calculation of isotope patterns in tandem mass
438 spectrometry, *Rapid Commun. Mass Spectrom.* 22 (2008) 2707–2714. doi:10.1002/rcm.3668.
- 439 [21] J.I. García-Alonso, P. Rodríguez-González, IDMS procedures and calculation methods, in: *Isot. Dilution*
440 *Mass Spectrom.*, RSC Publishing, 2013: pp. 41–76
- 441 [22] P. Rodríguez-González, J.I. García Alonso, Recent advances in isotope dilution analysis for elemental
442 speciation, *J. Anal. At. Spectrom.* 25 (2010) 239. doi:10.1039/b924261a.
- 443 [23] Á. Castillo, E. Gracia-Lor, A.F. Roig-Navarro, J.V. Sancho, P. Rodríguez-González, J.I.G. Alonso, Isotope
444 pattern deconvolution-tandem mass spectrometry for the determination and confirmation of
445 diclofenac in wastewaters, *Anal. Chim. Acta.* 765 (2013) 77–85. doi:10.1016/j.aca.2012.11.033.
- 446 [24] World Anti-Doping Agency, Technical Document-TD2014DL Decision Limits for the Quantification of
447 Threshold Substances, (n.d.).
- 448 [25] Nordtest, Handbook for Calculation of Measurement Uncertainty in Environmental Laboratories,
449 (2012).
- 450 [26] J. Kragten, Tutorial review. Calculating standard deviations and confidence intervals with a
451 universally applicable spreadsheet technique, *Analyst*. 119 (1994) 2161. doi:10.1039/an9941902161.
- 452